

# eOrder

## Online Laboratory Ordering

---

### **MT EVOLUTION User Guide – Extras**

## 1 TABLE OF CONTENTS

---

<b>ONLINE LABORATORY ORDERING</b>	<b>0</b>
<b>MT EVOLUTION USER GUIDE – EXTRAS</b>	<b>0</b>
<b>1 INTRODUCTION</b>	<b>2</b>
<b>2 ON SCREEN PROMPTS</b>	<b>2</b>
<b>2.1 Inappropriate Tests</b>	<b>2</b>
<b>2.2 Previous Results Available Indicator</b>	<b>3</b>
<b>2.3 Clinical Details required</b>	<b>3</b>
<b>2.4 Instructions for Patients</b>	<b>4</b>
<b>3 LINK TO SPECIMEN COLLECTION GUIDE</b>	<b>4</b>
<b>4 CONFIGURING THE MY TAB</b>	<b>5</b>

## 1 Introduction

This user guide explains some of the useful features available in the eOrder system.

## 2 On Screen Prompts

The Test details screen provides a number of on-screen reminders or prompts.

### 2.1 Inappropriate Tests

1. Tests which are not usually appropriate for the patient you have selected are identified in the form.
2. For example, this patient is Female and therefore the PSA test is greyed out.

The screenshot shows a grid of test categories with checkboxes. The 'Biochemistry' section includes tests like Lipid Test, Liver Function Tests, Alkaline Phosphatase, GGT, ALT, TSH, Electrolytes (NA/K), Creatinine, Uric Acid, Calcium/phosphate, PSA (highlighted in red and greyed out), LH, FSH, Progesterone, Oestradiol, and CVRA profile. Other sections include Haematology (Com, Iron, Ferrit, Vitan, Serui, INR I), Antenatal (1st A, 1st A, Subs, Glucc, HCG), Immunology (CRP, Rheu, Coeli), and Diabetes.

3. In this example, HbA1C is shown in a pale blue colour.

The screenshot shows the 'Diabetes' section with checkboxes for Haemoglobin A1c (highlighted in red and pale blue), Urine Albumin/Creatinine, Glucose, and Glucose Tolerance \*appt. Below this is the 'Critical Tests' section.

4. This is to advise that an order has been placed for this patient within the recommended frequency – in this case within the last 90 days.
5. Hovering the mouse over the test will provide information about the test itself and the reasons why it is showing in the way that it does.


The screenshot shows a tooltip for the 'Haemoglobin A1c' test. The tooltip text reads: 'This item is within its minimum reorder interval. Days since it was last ordered : 21'. Below this, it says: 'Please record if patient has a known Haemoglobinopathy and what type. If patient had a blood transfusion or venesection(s) in the last 3 months a fasting glucose is more appropriate'. The background shows the test selection interface with various tests listed.


6. However, you can still order this test if clinically indicated, using the Additional tab.


## 2.2 Previous Results Available Indicator

1. Where a test is shown with a blue arrow next to it, there are previous results for this test.




















**Biochemistry**

  Lipid Test

  Liver Function Tests

  Alkaline Phosphatase

2. Click on the blue arrow.
3. The previous tests screen will open and show the status, together with clinical information.

Existing results					
General Chemistry					
◀ Previous results					
					
	06/06/17 15:39	28/06/17 11:39	13/11/17 14:03	20/11/17 17:46	20/12/17 07:00
Sodium	 pending	 pending			 142
Potassium	 pending	 pending			 5.3
Creatinine	 pending	 *pending	38	20	 107
eGFR			> 90	> 90	 50
General Chemistry					
Fasting status	 Non-fasting				
General Chemistry 20/12/17 07:00					
Potassium reference interval is for serum samples. Potassium in plasma samples may be up to 0.3 mmol/L lower.					
An e-GFR result in the range 45-59 ml/min/1.73m2 suggests moderately impaired renal function, stage 3a CKD. Refer <a href="http://www.kidney.org.au">www.kidney.org.au</a> .					
Estimated GFR is calculated from the CKD-EPI equation.					
Caution in interpretation is required in non-Caucasians, the elderly, patients with extremes of body weight, oedema, rapidly changing creatinine and in pregnancy.					
General Chemistry 20/11/17 17:46					
An e-GFR result $\geq 90$ ml/min/1.73m2 falls in the range found for healthy adults. Refer <a href="http://www.kidney.org.au">www.kidney.org.au</a> .					
Estimated GFR is calculated from the CKD-EPI equation.					
General Chemistry 13/11/17 14:03					
An e-GFR result $\geq 90$ ml/min/1.73m2 falls in the range found for healthy adults. Refer <a href="http://www.kidney.org.au">www.kidney.org.au</a> .					
Estimated GFR is calculated from the CKD-EPI equation.					

## 2.3 Clinical Details required

1. If a test requires specific clinical indicators to be included, the eOrder form will prompt.
2. In this example, the ESR test has been selected and the requestor must include the clinical indicator to inform the laboratory of the reason for the test request.

**Please provide some additional information for this item.**

Item **ESR**


Clinical indication required for testing

Clinical indication

[Click here for ESR Clinical Update](#)

## 2.4 Instructions for Patients

1. Instruction to patients on how to collect the sample are printed on the order form, as shown.

Order No. EC00006117		<b>WELLINGTON SCL</b>	
		<p>Test results are available to health professionals involved in your care via a secure online database known as Eclair. You can choose to restrict sharing of your test results by calling 04 5868 571, however this may result in some tests being retaken.</p>	
26/07/18 15:34			
<p>Collection rooms at: <a href="http://www.wellingtonscl.co.nz">www.wellingtonscl.co.nz</a> or phone <b>04 381 5900</b> for opening hours information. Note: The last 10 minutes of every day is reserved for drop off and urgent samples only.</p>			
NHI : ZZZ9994	Address : TEST PATIENT FOR AUCKLAND DHB		
Surname : LABTEST	TE ATATU PENINSULA		
Given : JOHN	AUCKLAND		
DOB : 16/08/60 Sex: Male	0610		
Ethnicity : Asian not further defined	Phone : 0275551234(M) 1234555(H) 5551234(B)		
Eligible for publicly funded services?: Yes	Patient opt off laboratory record?: No		
Requester : Dr DOOLITTLE Barnaby (96ZZZZ)			
Address : Your Medical Practice			
Priority: Routine			
Fasting: No			
<p><b>Patient Information :</b>  <b>Patient instructions for collection of MID-STREAM URINE (MSU) MALE</b>                  (1) Clean around the urinary opening and genital area with a piece of toilet paper moistened with water.                  (2) Draw back the foreskin. Dry the area.                  (3) Pass a little urine into the toilet, then without stopping collect some urine 'mid stream' into the plastic collection punnet.                  (4) Finish passing urine into the toilet. Do not collect the last stream.                  (5) Pour the urine from the collection punnet into the specimen container and screw the lid on firmly.                  (6) Discard the collection punnet.                  (7) Write your full name, date of birth, and date and time of collection on the container label and place container in the delivery bag with the request form in the front pocket.                  (8) Store the sample in fridge if possible. Otherwise keep it in a cool place. Deliver to the laboratory as soon as possible.</p>			
Clinical details:			
Testing requested:			
<b>Urine Microbiology</b> • Urine site Mid Stream Urine			
Specimens to be collected (Tube, source)			
<b>Random Urine Container, Urine</b>			
<p><b>IMPORTANT INFORMATION FOR PATIENTS PLEASE READ:</b>                  Your medical centre will always contact you if there are significant results that require follow-up.                  If you feel you are not getting better or your health is deteriorating please contact your medical practice.</p>			

## 3 Link to Specimen Collection Guide

1. The eOrder web form links directly to the laboratory system and provides access to the Pathology Specimen Collection Guide.
2. This enables you to look up the cost of tests and also the collection methods and sample types if you are collecting a sample in your own practice.
3. In the left panel of the eOrder form you will see a link in bold black type.

In the left panel of the eOrder form you will see a link in bold black type.

for this order

Always create a Task

Ask every time

**Specimen Collection Guide**

4. The actual wording varies according to region.
5. Click on the link.

- In the screen which opens, type the name of the test.

A search input field containing the text 'Vitamin D'. To the right of the input field are two buttons: a grey 'x' button for clearing the search and a dark grey search button with a white magnifying glass icon.

- Then click on the Search button on the right.
- In the list which is displayed, click on the item you need.

A list of search results for 'Vitamin D'. The items are:
 

- 25-hydroxyvitamin D refer Vitamin D
- dihydroxyvitamin D (funded only) refer Calcitriol
- Vitamin D
- Vitamin D (non-funded)
- Vitamin D3 refer Vitamin D
- Vitamin D3 (non-funded) refer Vitamin D (non-funded)

- The item is displayed with cost and collection information.


Detailed view for 'Vitamin D (non-funded)'. The page is divided into several sections:

- General Information**
  - Name:** Vitamin D (non-funded)
  - Price (GST incl.):** \$53.50
  - Urgent:** No
  - Funding Type:** Not Funded
  - Funding Notes:**
    - This test is for ineligible patients or requests that do not meet the funding criteria.
    - Patient must pay at time of collection unless request form indicates charge to practice.
- Aliases**
  - 25 Hydroxy Vitamin D (non-funded)
  - 25 OH Vitamin D (non-funded)
  - Calciferol 25 OH (non-funded)
  - Cholecalciferol (non-funded)
  - Vitamin D3 (non-funded)
- Sample Types**
  - Preferred:** SST (Gold) x 1
  - Alternate:**
    - Microtainer SST (Gold) x 1
    - Plain (Red) x 1
    - Microtainer Plain (Red) x 1
- Specimen Collection**
- Department:** Biochemistry


## 4 Configuring the My Tab.

- The My Tab enables you to create your own groups of frequently ordered tests which means you can select all the tests with a single tick.
- This screen is user specific. The settings you create are personal to you and not shared with other members of your team.
- The eOrders team can copy groups automatically from one person's My Tab to the rest of the team.


- If you would like this done, please send the name of the clinician who has set up the My Tab AND their HPI/CPN number or NZMC/NZNC number to [helpdesk@eorder.co.nz](mailto:helpdesk@eorder.co.nz)

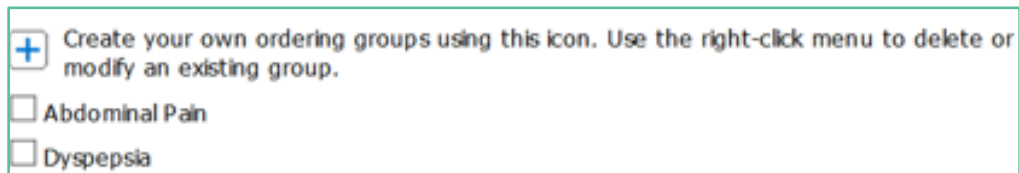


- You can add any tests which are available on the eOrder web form.
- If you are unable to find the test you require, please send a request to [helpdesk@eorder.co.nz](mailto:helpdesk@eorder.co.nz) to have it added to the Additional My Tab Tests group.
- The My Tab is user specific. Each user needs to set it up for him/herself.
- For this reason, it is often more efficient for the practice to send the list of test groups to the eOrder team for setup for ALL users.
- Click on the blue cross to open the Ordering Group form.
- Type the name of the test group in the Ordering Group Name field.
- The Display position controls the order in which your groups will be listed on the page. Pink infills show a group at that position already.




- To add tests to your group, type a few characters of the test name into the Search field and click on the Search button.

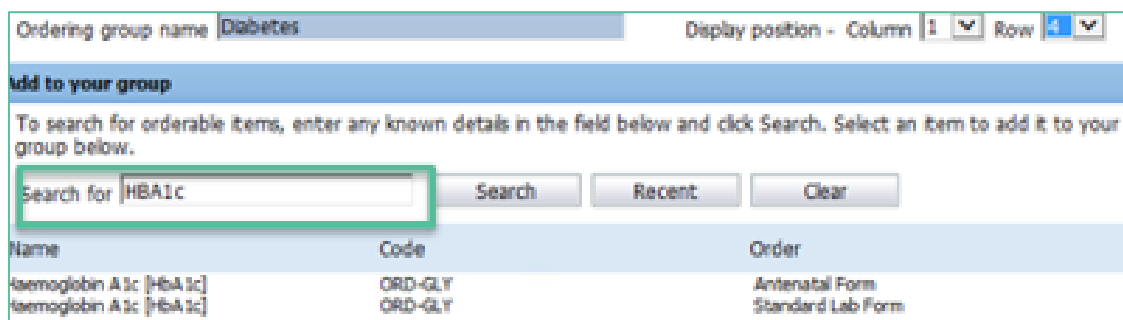

- To add an item to your group click on it. It will then be displayed in the lower pane. (Group Contents).

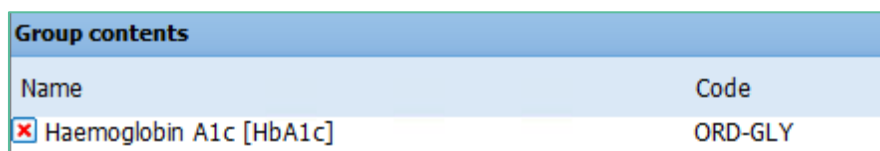

- Continue adding until your group is complete. Then click on the Save and Close button at the bottom of the screen.
- You can hover over your group to see the tests included in it.
- If you need to edit the group, right-click on the last letter of the group title and select the Edit option.



17. Click on the Red Cross to delete an item from the group.

Group contents	
Name	Code
<input checked="" type="checkbox"/> Complete Blood Count	ORD-CBC
<input checked="" type="checkbox"/> Ferritin	ORD-FER
<input checked="" type="checkbox"/> Liver Function Tests	ORD-LFT

18. Add extra tests exactly as before.

19. To Delete an Order group, right click and choose Delete.

20. When you make your selection of tests using the My Tab, the tests are automatically ticked in the tabs where these orders are located.

Further information can be found in the two companion user guides –

**Results and Amendments** and **Extras**

As well as the **FAQs** section on the eOrder website.