



## Online Laboratory Ordering

---

User Guide – How to order labtests online in Medtech32 /

### **Patient Mismatch**

# TABLE OF CONTENTS

---

<b>1</b>	<b>DOCUMENT PROPERTIES .....</b>	<b>2</b>
1.1	PURPOSE .....	2
1.2	SCOPE .....	2
1.3	DEFINITIONS.....	2
<b>2</b>	<b>EORDER OVERVIEW .....</b>	<b>3</b>
<b>3</b>	<b>PRE-REQUISITES.....</b>	<b>4</b>
3.1	ACCESS FOR USERS.....	4
3.2	COMPUTER SETUPS.....	4
<b>4</b>	<b>PATIENT MISMATCH .....</b>	<b>5</b>
<b>5</b>	<b>SUPPORT.....</b>	<b>6</b>
5.1	SUPPORT CONTACT DETAILS .....	6
5.2	EORDERS HELPDESK HOURS .....	6
	<b>REFER TO USER GUIDE APPENDIX A FOR ADDITIONAL INFORMATION.....</b>	<b>6</b>

# 1 Document Properties

## 1.1 Purpose

The purpose of this document is to explain how to order laboratory tests on line using the eOrder web form.

## 1.2 Scope


This information applies to any Healthcare Professionals who use the **Medtech32** Practice Management System.

## 1.3 Definitions

<b>PMS</b>	Practice Management System (Medtech32)
<b>eOrder</b>	Web ordering form
<b>Icon</b>	A picture on screen, which launches a task

## 2 eOrder Overview

- 2.1.1 Ordering laboratory tests online using the eOrder web form in **Medtech32** is very similar to the current process.
- 2.1.2 The eOrder web form has been designed to present the most commonly requested tests in the primary screen, to facilitate the requestor's workflows.
- 2.1.3 Results are delivered back to the Medtech32 inbox via Healthlink just as they are now. However, eOrder also provides results and status reports for **any** orders placed through Healthscope, providing a more comprehensive view of the patient's diagnostic test history.
- 2.1.4 Frequently ordered groups of tests can be organised into a one-click screen, called the My Tab.
- 2.1.5 The flowchart shows how the eOrder progresses from GP to laboratory and how results return to the GP.

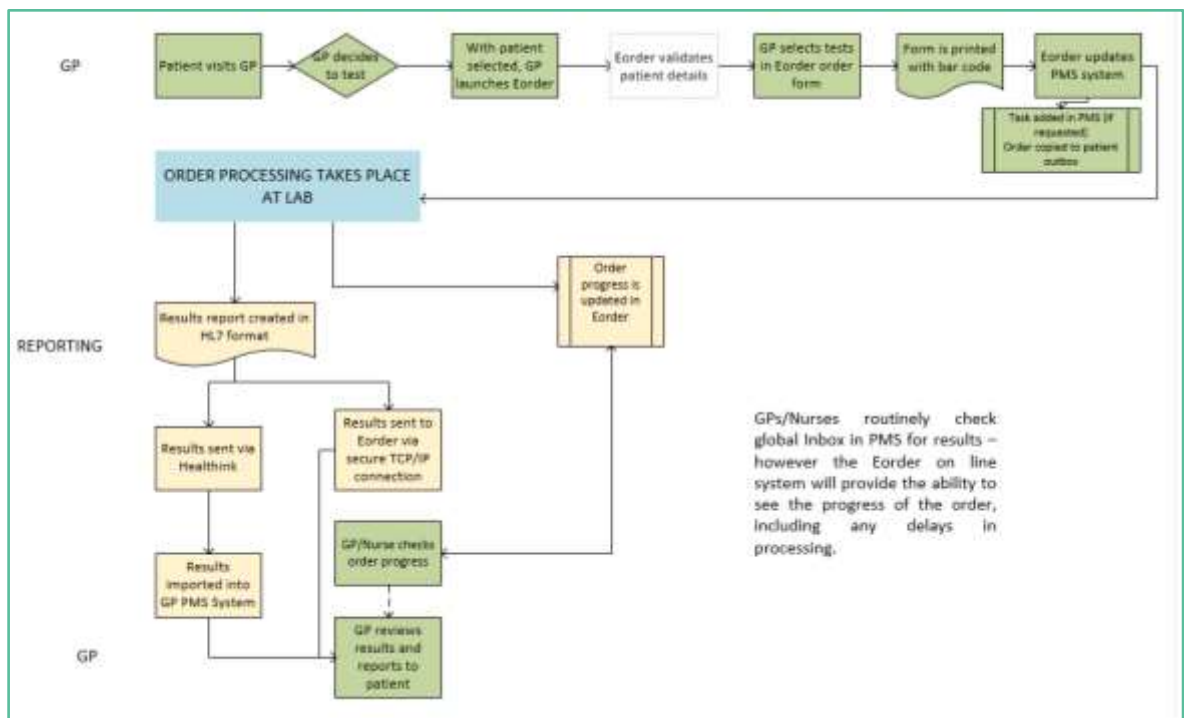

## 3 Pre-Requisites

### 3.1 Access for Users

- 3.1.1 The eOrder system is a secure system. Access is strictly controlled and limited to Healthcare Professionals.
- 3.1.2 The practice must supply to Healthscope the following information so that it can be set up in the eOrder system:
  - 3.1.3 The practice name and HPI (Organisation) number
  - 3.1.4 The names and HPI/CPN numbers of all healthcare professionals requiring access.
  - 3.1.5 A Practice representative must also sign an Acceptable Use Agreement to confirm that all users of the eOrder system understand and accept the Terms and Conditions.

### 3.2 Computer Setups

- 3.2.1 The eOrder system needs to be set up, configured and tested at the practice.
- 3.2.2 Some changes to a user's computer settings may be required.
- 3.2.3 All setup instructions and requirements are explained in Appendix A.

## 4 Patient Mismatch

- 4.1.1 Because the eOrder system is directly connected to the Laboratory system, when you start to place an order, it will check to see if a patient is already known to the laboratory system.
- 4.1.2 If it finds a similar patient with discrepancies, the eOrder form will ask you to confirm the details.
- 4.1.3 In this example, the patient in Medtech32 is being matched to a patient known to the eOrder system based on the NHI number.

The screenshot shows a 'Create Order' window with a warning icon and text: 'The patient information in your PMS conflicts with the information in Eclair for this NHI.' Below this, there are two tables comparing patient information from PMS and Eclair.

Information from your PMS:

NHI	First name	Last name	Date of birth	Sex	Age	Address
ZZZ9994	MICKEY	MOUSE	26 Jul 1980	M	38y	24 Justin Place, TE ATATU PENINSULA, AUCKLAND, 0610

Information from Eclair:

NHI	First name	Last name	Date of birth	Sex	Age	Address
ZZZ9994	JOHN	LABTEST	16 Aug 1960	M	57y	TEST PATIENT FOR AUCKLAND DHB, TE ATATU PENINSULA, AUCKLAND, 0610

There is a difference in the patient's date of birth.  
Value from your PMS: **26/07/80**  
Value already in Eclair: **16/08/60**

At the bottom right, there are three buttons: 'Use PMS Details' (highlighted with a green box), 'Use Eclair Details', and 'Cancel'.

- 4.1.4 To continue, you would confirm that the details in Medtech32 are correct, then click on the "Use PMS details" button in the bottom right hand corner.
- 4.1.5 The details held in the eOrder system will update to match what is in Medtech32.

## 5 Support

### 5.1 Support Contact Details

For support and assistance please contact our eOrder team

Website: [www.eorder.co.nz](http://www.eorder.co.nz)  
Phone: 0508 37 37 83  
Email: [helpdesk@eorder.co.nz](mailto:helpdesk@eorder.co.nz)  
[enquires@eorder.co.nz](mailto:enquires@eorder.co.nz)

### 5.2 eOrders helpdesk hours

Monday to Friday

7am – 6pm

**Refer to User Guide Appendix A for additional information**